


IMPACT VALUE OF AGGREGATE

1. Objective: The aggregate impact value gives a relative measure of the resistance of an aggregate to sudden shock or impact, which in some aggregates differs from its resistance to a slow compressive load.

2. Apparatus Required:

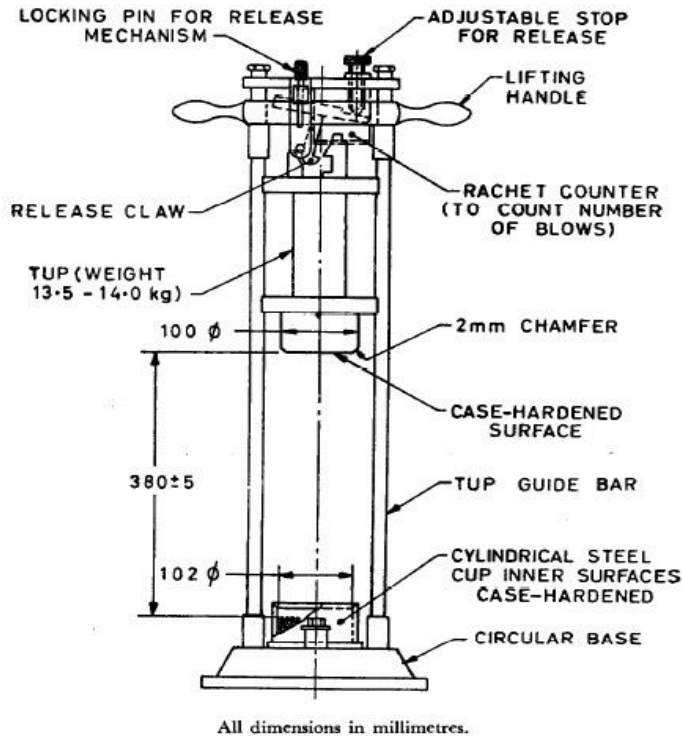

1. Balance: Balance should be accurate upto 1 g

2. Sieves: Sieves required are 12.5, 10.0 and 2.36 mm

3. Impact Testing machine: Weight of hammer is 13.5 to 14.0 kg and Height of Fall is 380+/-5 mm

Fig. 1: Impact Testing Machine

3. Reference: IS 2386(Part 4):1963 Methods of Test for Aggregates for Concrete- Mechanical Properties. Reaffirmed- Dec 2002

4. Procedure: The test sample shall consist of aggregate the whole of which passes a 12.5 mm IS Sieve and is retained on a 10 mm IS Sieve. The aggregate comprising the test sample shall be dried in an oven for a period of four hours at a temperature of 100°C to 110°C and cooled.

1. The measure shall be filled about one-third full with the aggregate and tamped with 25 strokes of the rounded end of the tamping rod. The net weight of aggregate in the measure shall be determined to the nearest gram (Weight A).

2. The impact machine shall rest without wedging or packing upon the level plate, block or floor, so that it is rigid and the hammer guide columns are vertical.
3. The cup shall be fixed firmly in position on the base of the machine and the whole of the test sample placed in it and compacted by a single tamping of 25 strokes of the tamping rod.
4. The hammer shall be raised until its lower face is 380 mm above the upper surface of the aggregate in the cup, and allowed to fall freely on to the aggregate. The test sample shall be subjected to a total of 15 such blows each being delivered at an interval of not less than one second.
5. The crushed aggregate shall then be removed from the cup and the whole of it sieved on the 2.36 mm IS Sieve until no further significant amount passes in one minute. The fraction passing the sieve shall be weighed to an accuracy of 0.1 g (Weight. B).
6. The fraction retained on the sieve shall also be weighed (Weight C) and, if the total weight (C+B) is less than the initial weight (Weight A) by more than one gram, the result shall be discarded and a fresh test made. Two tests shall be made.

5. Calculation: The ratio of the weight of fines formed to the total sample weight in each test shall be expressed as a percentage, the result being recorded to the first decimal place:

$$\text{Aggregate Impact Value} = (B/A) \times 100$$

Where,

A = weight in g of saturated surface dry sample,

B = weight in g of fraction passing through 2.36 mm IS Sieve